

Accuracy of Computer-Aided Dynamic Navigation Compared to Computer-Aided Static Navigation for Dental Implant Placement: An In Vitro Study

Alfonso Mediavilla Guzmán¹, Elena Riad Deglow¹, Álvaro Zubizarreta-Macho^{1,*}, Rubén Agustín-Panadero² and Sofía Hernández Montero¹

¹ Department of Implant Surgery, Faculty of Health Sciences, Alfonso X el Sabio University, 28691 Madrid, Spain

² Department of Stomatology, Faculty of Medicine and Dentistry, University of Valencia, 46010 Valencia, Spain

Abstract: Aim: To analyze the accuracy capability of two computer-aided navigation procedures for dental implant placement. Materials and Methods: A total of 40 dental implants were selected, which were randomly distributed into two study groups, namely, group A, consisting of those implants that were placed using a computer-aided static navigation system ($n = 20$) (guided implant (GI)) and group B, consisting of those implants that were placed using a computer-aided dynamic navigation system ($n = 20$) (navigation implant (NI)). The placement of the implants from group A was performed using surgical templates that were designed using 3D implant-planning software based on preoperative cone-beam computed tomography (CBCT) and a 3D extraoral surface scan, and the placement of group B implants was planned and performed using the dynamic navigation system. After placing the dental implants, a second CBCT was performed and the degree of accuracy of the planning and placement of the implants was analyzed using therapeutic planning software and Student's t-test. Results: The paired t-test revealed no statistically significant differences between GI and NI at the coronal ($p = 0.6535$) and apical ($p = 0.9081$) levels; however, statistically significant differences were observed between the angular deviations of GI and NI ($p = 0.0272$). Conclusion: Both computer-aided static and dynamic navigation procedures allow accurate implant placement.

Keywords: computer-assisted surgery; image-guided surgery; implantology; navigation system; real-time tracking

1. Introduction

Dental implant placement has recently emerged as a predictable treatment option to restore edentulous patients [1]. Nevertheless, some complications are attributed to this technique, including cortical or dental perforations and damage to particular anatomical structures, such as the inferior alveolar nerve or the maxillary sinus, due to implant malpositioning [1,2]. Recently, dental implant placement using image data-based navigation has been introduced into the field of dental surgery in an attempt to improve the accuracy of dental implant placement and avoid potential risks associated with this therapeutic procedure [3]. This surgical approach was developed based on preoperative cone-beam computed tomography (CBCT) scanning and specific 3D implant-planning software, thereby allowing for

accurate implant placement [4]. Generally speaking, there are two types of computer-assisted surgical implant placement system techniques, namely, static navigation and dynamic navigation.

Static navigation systems require the use of surgical templates to guide the drilling process. Dynamic navigation systems recognize and track the position of optical reference markers placed over the patient and surgical instruments by means of a tracking system array. Both navigation techniques have been widely analyzed, demonstrating high accuracy levels for dental implant placement [1,3,5,6]. Static navigation systems have a mean horizontal deviation at the coronal entry point and apical endpoint of 1.2 mm (1.04–1.44 mm) and 1.4 mm (1.28–1.58 mm), respectively, and a mean angular deviation of 3.5 (3.0–3.96) [7]. However, dynamic navigation systems demonstrated lower deviation values at the coronal entry point (0.71 0.40 mm), apical endpoint (1.00 0.49 mm), and angular deviation (2.26 1.62) [8], but these values have not yet been compared.

The aim of this work was to analyze and compare the accuracy of dental implant placement via static and dynamic navigation systems, with a null hypothesis (H0) stating that there would be no difference between the static and dynamic navigation systems with regard to the accuracy of dental implant placement.

2. Materials and Methods

2.1. Study Design

A randomized controlled experimental trial was conducted in accordance with the principles defined in the International Organization for Standardization (ISO 14801). The study was performed at the Dental Centre of Innovation and Advanced Specialties at Alfonso X El Sabio University (Madrid, Spain) between January and March 2019. This study was authorized by the Ethical Committee of the Faculty of Health Sciences, University Alfonso X el sabio, in December 2018.

2.2. Experimental Procedure

Forty dental implants (BioHorizons, Birmingham, AL, USA) were placed in tooth positions 2.4 and 2.6 (4.6 mm 12 mm, conical wall and internal taper) in twenty standardized polyurethane models of partially edentulous upper jaws (Sawbones Europe AB, Malmö, Sweden) based on one obtained from a real clinical case. The dental implants were randomized (Epidat 4.1, Galicia, Spain) and assigned to one of two study groups: group A, consisting of dental implants that were placed using a computer-aided static navigation system (NemoStudio^{fi}, Nemotec, Madrid, Spain) (n = 20) (guided implant (GI)) and group B, consisting of dental implants that were placed using a computer-aided dynamic navigation system (Navident, ClaroNav, Toronto, Canada) (n = 20) (navigation implant (NI)). The dental implants were first placed in tooth position 2.4, followed by position 2.6, in consideration of a real situation.

The GI jaw models were submitted for a preoperative CBCT scan (WhiteFox, Satelec, Merignac, France) with the following exposure parameters: 105.0 kV peak, 8.0 mA, 7.20 s, and a field of view of 15 mm 13 mm. Afterward, the ten jaw models assigned to the GI study group were submitted for a 3D-extraoral surface scan (EVO, Ceratomic, Protechno, Girona, Spain). Datasets obtained from the digital workflow were uploaded into 3D implant-planning software (NemoStudio^{fi}) to design virtual templates for GI implant placement. The 3D surface scan and CBCT data were matched by aligning the key points present in the partially edentulous upper jaw models. A virtual implant drill was designed with a diameter and length of 4.6 and 12 mm, respectively, as per the measurements of the selected implant (Figure 1A,B). After designing the virtual templates (Figure 1C,D), they were fabricated using the stereolithography technique (ProJet 6000, 3D Systems, Rock Hill, SC, USA) (Figure 1E), except for the 5 mm stainless steel cylinders, which were manually attached to the templates. The templates fit the model and did not need further adjustments.

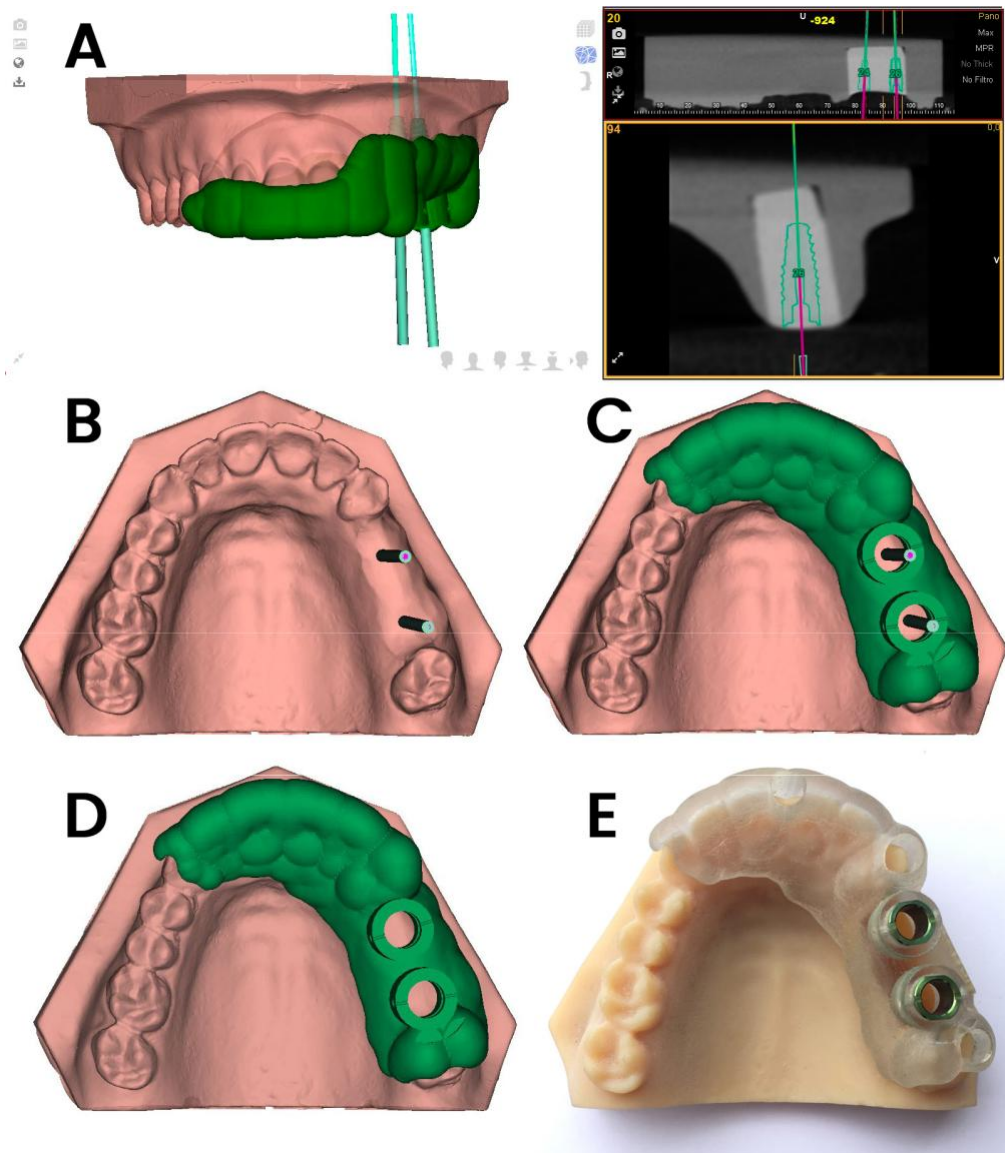


Figure 1. A–C Dental implant planning with the computer-aided static navigation system using a cone-beam computed tomography (CBCT) scan (green lines); (C,D) virtual template design according to the planned virtual dental implant placement; (E) manufactured stereolithography template fixed to the planned virtual dental implant placement; (E) manufactured stereolithography template fixed to the planned virtual dental implant placement.

The NI jaw models were submitted to a preoperative CBCT scan prior to placement off the thermoplastic template ((Navident, ClaroNav,av, Toronto, ON, Canada) that includes a radiographic marker and an attached handle with a black and white tag, which was fixed to the over dental surface of the teeth of the CBCT datasets. CBCT datasets imported were imported into the planning treatment software-planning on a mounted computer laptop in mobile computer unit (Navident, in mobile ClaroNav, unit (Navident, Toronto, ClaroNav, Canada) Toronto, simulate Canada dental) implant to simulate placement of dental implant (Figure 2 placement A). Another (Figure 2 A) .white Another drill bit tag was attached to the tag and piece was attached. Both optical reference. Both markers optical were reference calibrated markers and recognized were calibrated by the optical triangulation system composed of tracking of system stereoscopic composed of motion of tracking stereoscopic cameras motion which tracking guided camera the drilling which process guided at the planned drilling angle, process pathway, the

planned depth angle, in real pathway, time. Socket and depth drilling in was real performed time. Socket with drilling a was (Ref. performed TSD2041, BioHorizons) with a drill (Ref. TSD2041, was monitored BioHorizons) on the and laptop was connected to a computer containing using the laptop computer computer-aided dynamic navigation system (Figure 2B). navigation system (Figure 2B).

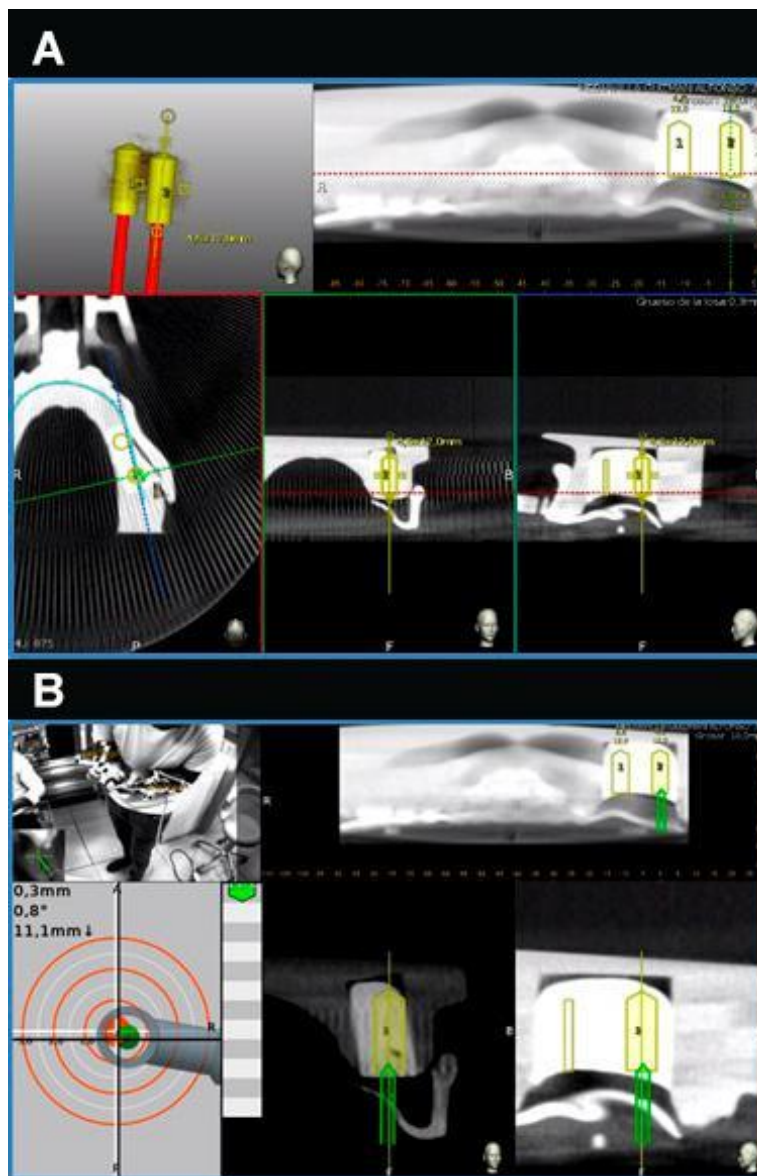


Figure 2. (A) Dental implant planning as seen in the treatment-planning software of the computer-2. (B) Dental implant placement as seen in the treatment-planning software the computer-aided dynamic navigation system (yellow cylinders) and (B) dental implant placement (green dynamic navigation system (yellow cylinders) at all planes and depths.

2.3. Measurement Procedure

Following the dental implant placement, postoperative CBCT scans were taken. Dental implant planning and postoperative CBCT scans of the study groups were uploaded into 3D implant-planning software (NemoScan, Nemotec, Madrid, Spain) and matched to analyze apical deviation, which was measured at the apical endpoint; coronal deviation, which was measured at the entry point; and angular deviation, which was measured at the apical endpoint. All noted deviations of all of the implants point; and angular deviation, which was measured the center of the cylinder. All noted deviations were evaluated and compared in the axial, sagittal, and coronal views (Figure 3A,B) using the same of all of the implants were evaluated and compared in the axial, sagittal, and coronal views (Figure 3A-B) using the same expertise operator. Results were expressed according to each position.

2.4. Statistical Analysis

Statistical analysis of all variables was carried out using SAS 9.4 (SAS Institute Inc., Cary, NC, USA). Descriptive statistics were expressed as mean and standard deviation (SD) values for quantitative variables and as absolute numbers and percentages for qualitative variables. Comparative analysis was performed by comparing the mean deviation values between planned and

J. Clin performed. Med. 2019 implant, 8,2123 placements using Student's *t*-test as the variables had a normal distribution. The 5 of 9 statistical significance was set at $p < 0.05$.

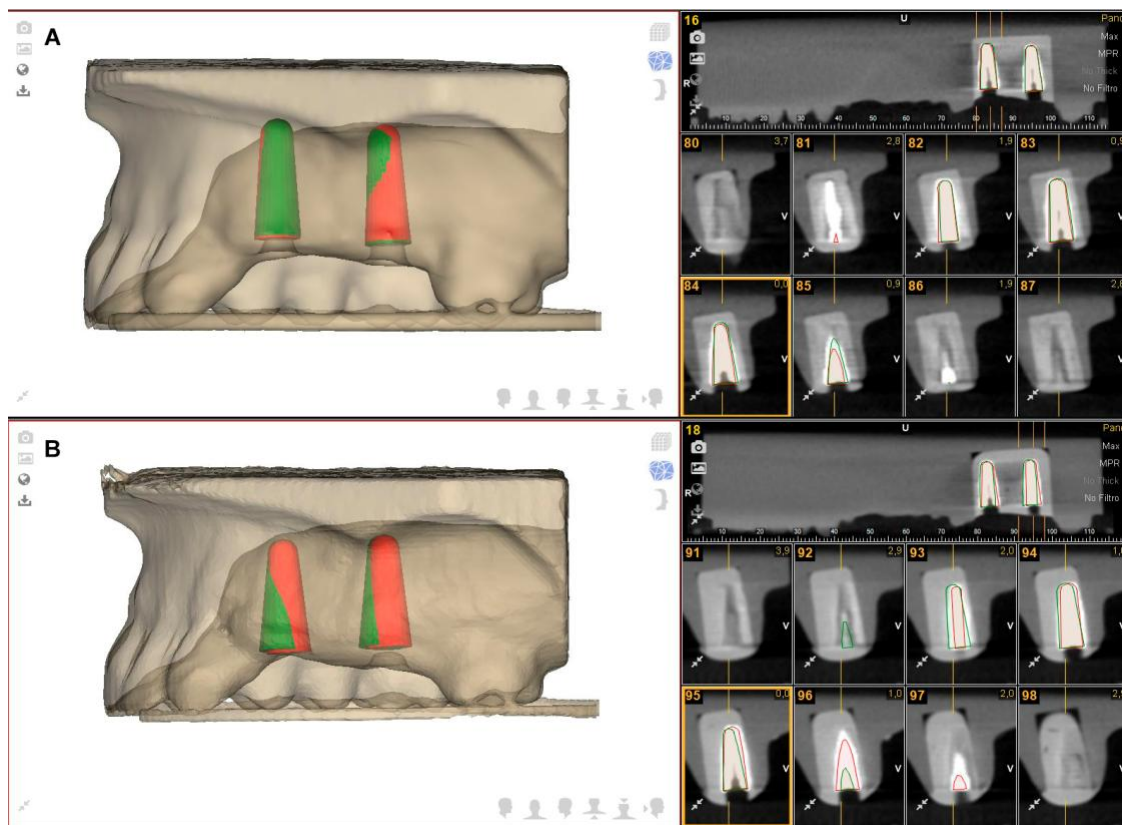


Figure 3. (A) Dental implant planning (green cylinders) and dental implant placement (red cylinders) using the computer-aided static navigation system and (B) the computer-aided dynamic navigation system.

2.43. .StatisticalResults Analysis

Statistical analysis of all variables was carried out using SAS 9.4 (SAS Institute Inc., Cary, NC, USA). Descriptive statistics were expressed as mean and standard deviation (SD) values for quantitative variables and as absolute numbers and percentages for qualitative variables. Comparative analysis of the GI (Figure 3A) and NI (Figure 3B) study groups, respectively (Figure 4). was performed by comparing the mean deviation values between planned and performed implant placements using Student's *t*-test as the variables at the apical had (mm), a normal coronal distribution (mm), and angular (°) statistical levels (guided significance was set implant at < 0.05 . static navigation system; navigation implant (NI): dynamic navigation system).

3. Results	n	Mean	SD	Minimum	Maximum
CORONAL	GI 20	0.78	0.43	0.20	1.70
Table 1 shows the mean NI and 20SD values. 0.85 Mean deviations 0.48 of 0.78 0.30 0.43 mm (min: 0.20 1.90 mm; max: 1.70 mm) and 0.85 0.48 mm GI (min: 0.30 mm; 1.20 max: 1.90 48mm) were observed 0.30 at the coronal 2.10 entry point					
APICAL	GI 20	2.95	1.48	0.60	5.20 *
of the GI (Figure 3A) and NI (Figure 3B) study groups, respectively (Figure 4).					
ANGULAR	GI 20	4.00	1.41	1.60	6.10
Table 1. Descriptive deviation values at the apical (mm), coronal (mm), and angular (°) levels (guided implant (GI): static navigation system; navigation implant (NI): dynamic navigation system).					

n	Mean	SD	Minimum	Maximum
---	------	----	---------	---------

CORONAL	GI	20	0.78	0.43	0.20	1.70
	NI	20	0.85	0.48	0.30	1.90
APICAL	GI	20	1.20	0.48	0.30	2.10
	NI	20	1.18	0.60	0.20	2.50
ANGULAR	GI	20	2.95	1.48	0.60	5.20 *
	NI	20	4.00	1.41	1.60	6.10

Figure 4. Box plots of the coronal deviations observed in the experimental groups. The horizontal lines in each box represent the median values (GI: static navigation system; NI: dynamic navigation system).

The paired *t*-test revealed no statistically significant differences between the coronal deviations of GI and NI ($p = 0.6535$). Mean deviations of 1.20 ± 0.48 mm (min: 0.30 mm; max: 2.10 mm) and 1.18 ± 0.60 mm (min: 0.20 mm; max: 2.50 mm) were observed at the apical endpoint of the GI (Figure 3A) and NI (Figure 3B) study groups, respectively (Figure 5). The paired *t*-test revealed no statistically significant differences between the coronal deviations and 1.18 ± 0.60 mm (min: 0.20 mm; max: 2.50 mm) were observed at the apical endpoint of the GI (Figure 3A) and NI (Figure 3B) study groups, respectively (Figure 5).

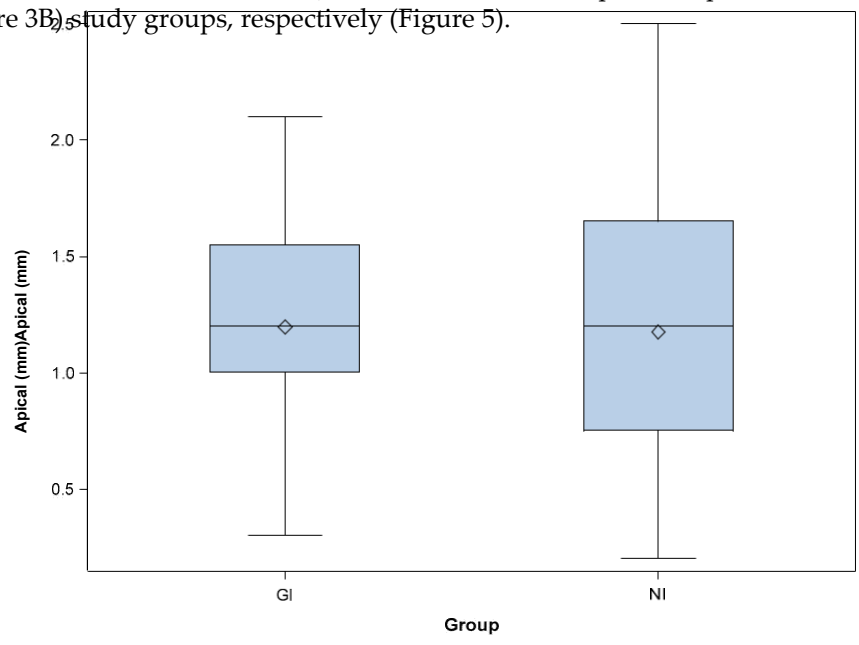


Figure 5. Box plots of the apical deviations observed in the experimental groups. The horizontal lines in each box represent the median values (GI: static navigation system; NI: dynamic navigation system).

The paired *t*-test revealed no statistically significant differences between the apical deviations of GI and NI ($p = 0.9081$). Mean deviations of 1.20 ± 0.48 mm (min: 0.30 mm; max: 2.10 mm) and 1.18 ± 0.60 mm (min: 0.20 mm; max: 2.50 mm) were observed at the apical endpoint of the GI (Figure 3A) and NI (Figure 3B) study groups, respectively (Figure 5). The paired *t*-test revealed no statistically significant differences between the apical deviations of GI and NI ($p = 0.9081$). Mean deviations of 1.20 ± 0.48 mm (min: 0.30 mm; max: 2.10 mm) and 1.18 ± 0.60 mm (min: 0.20 mm; max: 2.50 mm) were observed at the apical endpoint of the GI (Figure 3A) and NI (Figure 3B) study groups, respectively (Figure 5).

The paired *t*-test revealed no statistically significant differences between the apical deviations of

GI and NI ($p = 0.9081$). Mean deviations of $2.95^\circ \pm 1.48^\circ$ (min: 0.60° ; max: 5.20°) and $4.00^\circ \pm 1.41^\circ$ (min:

1.60°; max: 6.10°) were observed in the GI (Figure 3A) and NI (Figure 3B) study groups, respectively (Figure 6). The paired *t*-test revealed statistically significant differences between the angular J. Clin. Med. 2019, 8, 2123 7 of 9 deviations of GI and NI ($p = 0.0272$).

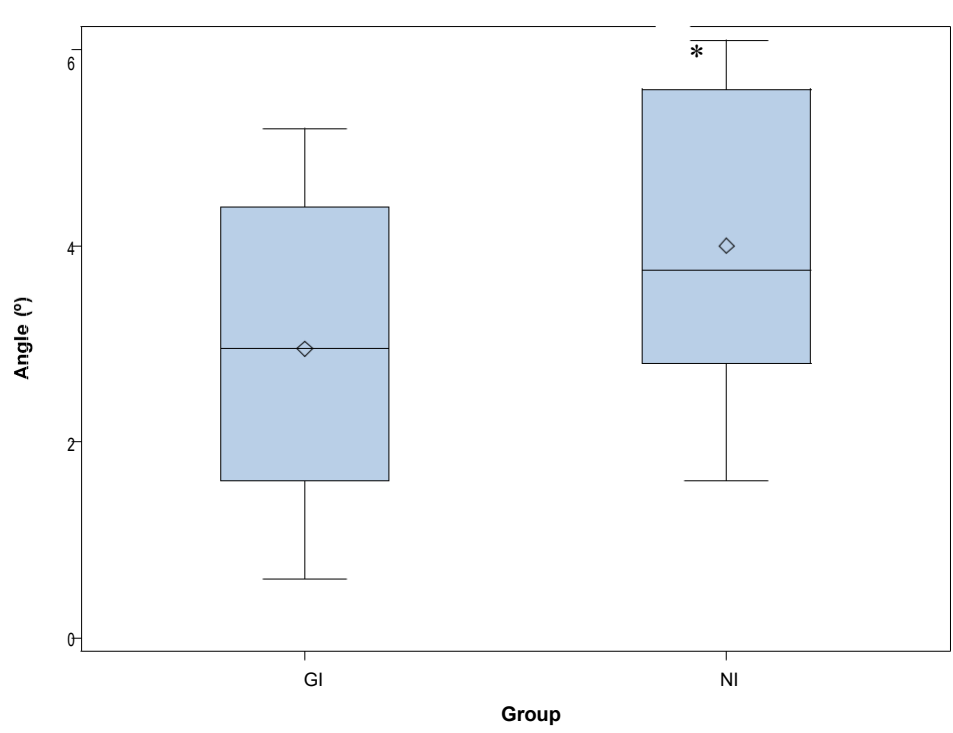


Figure 6. Box plots of the angular deviations observed in the experimental groups. The horizontal lines in each box represent the median values (GI: static navigation system; NI: dynamic navigation system).

4. Discussion

The results obtained in the present study rejected the null hypothesis (H_0) that stated that there would be no difference between computer-aided static and dynamic navigation systems with regard to the accuracy of dental implant placement.

The results obtained in the present study rejected the null hypothesis (H_0) that stated that there would be no difference between computer-aided static and dynamic navigation systems with regard to the precision and stability of the surgical template due to the use of models, which may have significantly the accuracy of surgical computer-aided navigation techniques has been widely evaluated and differed from what is encountered in a real clinical situation. In recent literature, precision and stability of the surgical template due to the use of models, which may have significantly the accuracy of surgical computer-aided navigation techniques has been widely evaluated and compared. Ho mann et al. [9] reported statistically significant differences in the accuracy of implant surgical computer-aided navigation techniques has been widely evaluated and compared. Hoffmann et al. [9] reported statistically significant differences in the accuracy of implant placement between with mean angular deviations of 4.2 ± 1.8 and $11.2 \pm 5^\circ$, respectively. Although the methods and selection criteria were computer-aided dynamic navigation system offered a greater degree of accuracy than manual implant placement, with mean angular selection criteria were slightly different from those used in the present study, implant placement using a computer-aided placement. Chang-Kai et al. [10] reported similar mean horizontal deviation values at the apical endpoint when navigation system (1.50 0.79 mm), and manual implant placement (2 0.79 mm). Higher angular deviation values at the apical endpoint when navigation system (1.35 0.55 mm), a computer-aided static Chang-Kai et al. [10] reported similar mean horizontal deviation values at the apical endpoint when navigation system (1.50 0.79 mm), and manual implant placement (2 0.79 mm). Higher angular deviation values at the apical endpoint when navigation system (1.35 0.55 mm), a computer-aided static deviation values were reported for the computer-aided dynamic navigation system (4.45 1.97), navigation system (1.50 0.79 mm), and manual implant placement (2 0.79 mm). Higher angular the computer-aided static navigation system (6.02 3.71), and manual implant placement (9.26 3.62).

deviation values were reported for the computer-aided dynamic navigation system ($4.45 \pm 1.97^\circ$), the The accuracy of implant placement with computer-aided navigation systems was shown to be better computer-aided static navigation system ($6.02 \pm 3.71^\circ$), and manual implant placement ($9.26 \pm 3.62^\circ$). than the degree of accuracy during manual procedures, but the angular deviation values were different

The accuracy of implant placement with computer-aided navigation systems was shown to be better from the present findings. The learning requirements of computer-aided dynamic navigation systems than the degree of accuracy during manual procedures, but the angular deviation values were might explain the differences between static and dynamic navigation systems [8]. Computer-aided different from the present findings. The learning requirements of computer-aided dynamic static navigation techniques performed using surgical templates prevent the need for drilling guidance navigation systems might explain the differences between static and dynamic navigation systems [8]. during surgery [1,3–5]. Therefore, implant placement accuracy depends directly on the design and

Computer-aided static navigation techniques performed using surgical templates prevent the need manufacturing process of the surgical template; if there is an inaccuracy during the fabrication process, for drilling guidance during surgery [1,3–5]. Therefore, implant placement accuracy depends directly this might lead to intraoperative complications [3]. On the other hand, computer-aided dynamic on the design and manufacturing process of the surgical template; if there is an inaccuracy during navigation systems allow for a direct view of the surgical field and provide clinicians with the ability to relocalize the position of an implant, if necessary [9,10]. In addition, these systems are particularly

useful in cases of limited mouth openings or treatments in the posterior region [1,8]. The main disadvantage of computer-aided dynamic navigation systems is the difficulty in keeping sight of the dynamic navigation system display during the surgical procedure. However, augmented reality devices could be used to display the virtual image of the computer-aided dynamic navigation system without losing sight of the surgical field [11,12]. Image-guided navigation systems demonstrated comparable accuracy rates regarding control of the depth, position, and angle of implants, which is necessary to avoid intraoperative surgical complications and poor positioning of implants, thereby compromising primary stability and immediate-loading restoration techniques [8,9,12]. In addition, they also avoid the wide excisions often needed to expose the implant platform after the healing period, and enable a minimally invasive transgingival approach to implant placement [1,12]. This is especially helpful in high-risk patients, such as cardiovascular patients taking anticoagulation medications or patients with edentulous, atrophic mandibles [12].

This study shows that computer-aided static and dynamic navigation procedures allow accurate dental implant placement. Nevertheless, further research is needed to determine the influence of the dental implant placement procedure on the accuracy of dental implant positioning and potential clinical complications.

5. Conclusions

In conclusion, within the limitations of this study, the results showed that computer-aided static and dynamic navigation procedures allow accurate implant placement. Nevertheless, it is mandatory to perform a CBCT scan and a 3D surface scan and to plan implant placement using specialized surgical planning software. Clinical trials are necessary to analyze the real behavior of these computer-aided navigation procedures.

Author Contributions: Conceptualization, R.A.-P. and S.H.M.; data curation, E.R.D.; formal analysis, A.M.G.; visualization, Á.Z.-M.

Funding: This research received no external funding.

Acknowledgments: The authors would like to thank Santiago López Martínez for his invaluable assistance in this study.

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Kaewsiri, D.; Panmekiate, S.; Subbalekha, K.; Mattheos, N.; Pimkhaokham, A. The accuracy of static vs. dynamic computer-assisted implant surgery in single tooth space: A randomized controlled trial. *Clin. Oral Implants Res.* **2019**, *30*, 505–514. [[PubMed](#)]
2. Herklotz, I.; Beuer, F.; Kunz, A.; Hildebrand, D.; Happe, A. Navigation in implantology. *Int. J. Comput. Dent.* **2017**, *20*, 9–19. [[PubMed](#)]
3. Widmann, G.; Bale, R.J. Accuracy in Computer-Aided Implant Surgery—A review. *Int. J. Oral Maxillofac. Implants* **2006**, *21*, 305–313. [[PubMed](#)]
4. Chasioti, E.; Sayed, M.; Drew, H. Novel Techniques with the Aid of a Staged CBCT Guided Surgical Protocol. *Case. Rep. Dent.* **2015**, *2015*, 439706. [[CrossRef](#)] [[PubMed](#)]
5. Lal, K.; White, G.S.; Morea, D.N.; Wright, R.F. Use of stereolithographic templates for surgical and prosthodontic implant planning and placement. Part II. A clinical report. *J. Prosthodont.* **2006**, *15*, 117–122. [[CrossRef](#)] [[PubMed](#)]

6. Jorba-García, A.; Figueiredo, R.; González-Barnadas, A.; Camps-Font, O.; Valmaseda-Castellón, E. Accuracy and the role of experience in dynamic computer guided dental implant surgery: An in-vitro study. *Med. Oral Patol. Oral Cir. Bucal* **2019**, *24*, 76–83. [[CrossRef](#)]
7. Tahmaseb, A.; Wu, V.; Wismeijer, D.; Coucke, W.; Evans, C. The accuracy of static computer-aided implant surgery: A systematic review and meta-analysis. *Clin. Oral Implants Res.* **2018**, *16*, 416–435. [[CrossRef](#)]
8. Stefanelli, L.V.; DeGroot, B.S.; Lipton, D.I.; Mandelaris, G.A. Accuracy of a Dynamic Dental Implant Navigation System in a Private Practice. *Int. J. Oral Maxillofac. Implants* **2019**, *34*, 205–213. [[CrossRef](#)]

9. Ho mann, J.; Westendor , C.; Gomez-Roman, G.; Reinert, S. Accuracy of navigation- guided socket drilling before implant installation compared to the conventional free-hand method in a synthetic edentulous lower jaw model. *Clin. Oral Implants Res.* **2005**, *16*, 609–614. [[CrossRef](#)] [[PubMed](#)]
10. Chen, C.K.; Yuh, D.Y.; Huang, R.Y.; Fu, E.; Tsai, C.F.; Chiang, C.Y. Accuracy of implant placement with a navigation system, a laboratory guide, and freehand drilling. *Int. J. Oral Maxillofac. Implants* **2018**, *33*, 1213–1218. [[CrossRef](#)] [[PubMed](#)]
11. Pellegrino, G.; Mangano, C.; Mangano, R.; Ferri, A.; Taraschi, V.; Marchetti, C. Augmented reality for dental implantology: A pilot clinical report of two cases. *BMC Oral Health* **2019**, *19*, 158–165. [[CrossRef](#)] [[PubMed](#)]
12. Gargallo-Albiol, J.; Barootchi, S.; Salomó-Coll, O.; Wang, H. Advantages and disadvantages of implant surgery. A systematic review. *Ann. Anat.* **2019**, *225*, 1–10. [[CrossRef](#)] [[PubMed](#)]

